

Chapter 45

A Novel Delay–Based GFSK Demodulator in 65 nm CMOS for Low Power Biomedical Applications

Meng Fu

University of Melbourne, Australia

Stan Skafidas

University of Melbourne, Australia

Iven Mareels

University of Melbourne, Australia

ABSTRACT

This article describes how, in recent years, with the development of microelectronics, implantable electronic devices have been playing a significant role in modern medicine. Examples of such electronic implant devices are, for instance, retinal prosthesis and brain implants. It brings great challenges in low power radio frequency (RF) and analog designs. This article presents a low power Gaussian frequency shift keying (GFSK) demodulator designed for Medical Implant Communications Service (MICS) band Receiver. This demodulator utilizes a novel structure that a wide IF range can be handled and presents the smallest $\Delta f/f$ ratio in any published GFSK demodulators. In theory the demodulation method can be applied to any RF frequency. The demodulator draws 550 μ A from a 1 V power supply. A maximum data rate of 400 Kbits/s can be achieved within the 300 KHz channel bandwidth defined by MICS. A simulated signal-to-noise ratio (SNR) of 15.2dB at AWGN channel is obtained to achieve 10^{-3} bit error rate (BER). This demodulator is fabricated on 65-nm CMOS and occupies 0.12mm² silicon area.

DOI: 10.4018/978-1-7998-1204-3.ch045


INTRODUCTION

The MICS band is an ultra-low power, unlicensed mobile radio service for implanted medical device. Ten 300 KHz channels are allocated at 402-405 MHz frequency band ("FCC Rules and Regulations," 2002). Implanted wireless device has a requirement of high reliability and ultra-low power consumption. Recent CMOS technology has enabled the design of reliable, low power and cost effective wireless transceiver. This demodulator is designed on 65nm technology under 1 V supply. It intends to be used for the epi-retinal prosthesis (Bionic Eye) to demodulate data for a 32x32 electrode array. In order to support these 1024 electrodes, a data rate more than 300 Kbps is required to make fully functional. Achieving high data rate and low power consumption from this limited 300 KHz bandwidth are challenges in the design of such system. So far, amplitude shift keying (ASK) and binary shift keying (BFSK) have been widely used in biomedical implants (Ghovanloo, Beach, Wise, & Najafi, 2002; Ghovanloo & Najafi, 2003). However, these two methods are not bandwidth efficient. This paper presents a demodulator that can work for both continuous phase BFSK and GFSK modulation schemes. Using GFSK, a data rate up to 400 Kbit/s is achieved within the given 300 KHz bandwidth. This demodulator is also immune to a frequency offset up to 4 MHz. A BER of 10^{-3} is obtained at SNR of 15.2 dB at the input.

DEMODULATOR ARCHITECTURE

The Architecture of the RF receiver is shown in Figure 1. The RF frequency is down converted from MICS band, 402-405MHz to around 5 MHz. A channel-select filter is used to reject the image and select the desired channel. Then the limiter amplifies the IF signal to rail-to-rail swing. Block diagram of proposed GFSK demodulator is shown in the dashed box of the figure. It consists of four blocks: delay line, delay flip-flop (DFF), gm-c low pass filter, and decision-making circuit. The delay element delays the IF input by approximate half the bit period. Then the DFF uses the delayed signal as the clock to sample the original signal. So the frequency information of GFSK signal is mapped into the density and width

Figure 1. Block diagram of receiver with the proposed GFSK demodulator

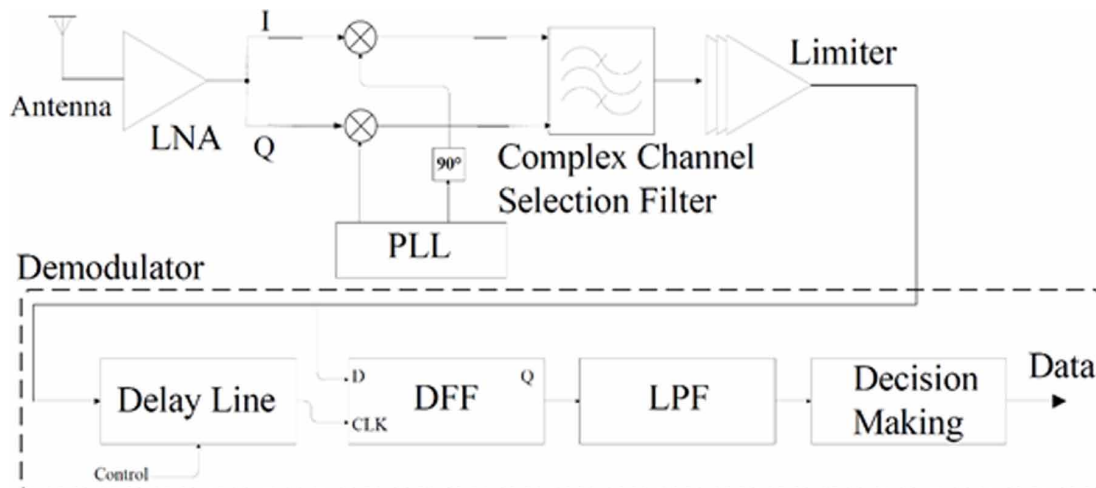

11 more pages are available in the full version of this document, which may be purchased using the "Add to Cart" button on the publisher's webpage:

www.igi-global.com/chapter/a-novel-delay-based-gfsk-demodulator-in-65-nm-cmos-for-low-power-biomedical-applications/243147

Related Content

Cardiovascular Risk Detection Through Big Data Analysis

Miguel A. Sánchez-Acevedo, Zaydi Anai Acosta-Chiand Ma. del Rocío Morales-Salgado (2020).

International Journal of Big Data and Analytics in Healthcare (pp. 1-11).

www.irma-international.org/article/cardiovascular-risk-detection-through-big-data-analysis/259985

Development of a New Means to Improve the Performance of Self-Organizing Maps

Vijaya Prabhagar Murugesanand Punniyamoorthy M. (2022). *International Journal of Data Analytics* (pp. 1-16).

www.irma-international.org/article/development-of-a-new-means-to-improve-the-performance-of-self-organizing-maps/307065

Loan Fraud Detection Using Machine Learning as a Data Mining Approach

Nabila Hamdoun (2022). *International Journal of Data Analytics* (pp. 1-10).

www.irma-international.org/article/loan-fraud-detection-using-machine-learning-as-a-data-mining-approach/309096

Big Data, Who Are You?

(2019). *Big Data Analytics for Entrepreneurial Success* (pp. 1-27).

www.irma-international.org/chapter/big-data-who-are-you/216179

Exploring Shared Work Values and Work Collaboration With a Network Approach: A Case Study From Italy

Aizhan Tursunbayeva, Stefano Di Lauroand Gilda Antonelli (2021). *Using Strategy Analytics to Measure Corporate Performance and Business Value Creation* (pp. 43-58).

www.irma-international.org/chapter/exploring-shared-work-values-and-work-collaboration-with-a-network-approach/285845